

Cat. # MK301

For Research Use

---

**TAKARA**

**TRACP & ALP Assay Kit**

---

Product Manual

v201607Da

## Table of Contents

I.	Description .....	3
II.	Introduction .....	3
III.	Components .....	4
IV.	Materials Required but not Provided .....	4
V.	Storage .....	4
VI.	Preparation of Reagents .....	5
VII.	Outline of Protocol .....	5
VIII.	Protocol .....	6
IX.	Experimental Examples .....	7
X.	References .....	13
XI.	Related Products .....	13

## I. Description

TRACP & ALP Assay Kit allows for simultaneous detection of 2 enzymes which are involved in bone metabolism. TRACP which is an osteoclast enzyme marker and ALP an osteoblast enzyme marker. TRACP & ALP Assay Kit has been designed for simple and quick detection of ACP (Acid phosphatase) and ALP (Alkaline phosphatase) through the use of pNPP (*p*-nitro-phenyl phosphate) substrate. The addition of tartaric acid into the ACP assay, allows for the detection of TRACP (tartrate-resistant acid phosphatase) activity. Since this kit utilizes an aqueous substrate, it enables quick activity quantification by measuring the absorbance of the reactant. In addition to this kit, TRACP & ALP double-staining Kit (Cat. #MK300) is also available using a non-soluble substrate. The appropriate kit can be selected depending on assay interest.

## II. Introduction

Phosphatase is an enzyme which hydrolyzes aliphatic and aromatic phosphate esters resulting in the release phosphates. The optimum pHs for alkaline and acid phosphatases activity are at alkaline and acid pHs, respectively. Acid phosphatases (ACP) are present in a variety of cells and tissues, such as prostate, liver, kidney, spleen, erythrocyte, platelet and osteoclast.<sup>1,2)</sup> In 1959, Burstone<sup>3)</sup> reported that potent acid phosphatase activity is found in the osteoclasts and alkaline phosphatase activity is found in the osteoblasts. Following this report, various research reports have been made on phosphatase activities associated with osteocytes. In addition to osteoclasts, hairy cells among blood cells are also known to have TRACP activity. The acid phosphatase activity of osteoclasts was shown to be of the type that retains phosphatase activity in the presence of tartrate (tartrate-resistant acid phosphatase : TRACP). The type of acid phosphatases that is inactivated in the presence of tartrate is called tartrate-sensitive acid phosphatase (TSACP). TRACP activity is now a requisite for osteoclasts.

Alkaline phosphatases (ALP) are membrane-bound glycoproteins and are classified into four types, i.e. intestinal, placental, placenta-like and tissue non-specific types. Among the tissue non-specific type alkaline phosphatases, the bone-specific isozyme is called bone type alkaline phosphatase. This enzyme is bound to the membrane of osteoblasts and functions to enhance osteogenesis by degrading pyrophosphates. Pyrophosphates inhibit crystallization at the calcification site and degrade organic phosphate esters to increase the inorganic phosphate concentration. Therefore, bone type alkaline phosphatase is known as a marker of osteogenesis in bone cycle metabolism. Since bone metabolism is composed of mutually balanced osteogenesis and bone resorption, simultaneous assay with two enzyme markers is useful.

**III. Components (for 500 reactions)**

- |  |           |
|--|-----------|
| (1) pNPP ( <i>p</i> -nitro-phenyl phosphate) Substrate [pNPP Substrate]<br>sufficient pNPP substrate is supplied to prepare 25 ml of<br>substrate solution which allows 500 assays in 50 $\mu$ l/well in<br>a 96-well plate. | 24 mg x 5 |
| (2) Extraction Solution<br>Physiological saline including 1 % NP-40<br>For solubilization of suspension and adherent cells   | 11 ml x 2 |
| (3) Sodium Tartrate Solution<br>0.5 M sodium tartrate buffer, pH 5.2<br>TRACP : Used for the detection of osteoclast marker through<br>the addition to the substrate solution  | 4 ml      |
| (4) Buffer for ACP<br>0.5 M Sodium acetate, pH 5.2   | 30 ml     |
| (5) Buffer for ALP<br>0.2 M Tris-HCl, pH 9.5, 1 mM MgCl <sub>2</sub>   | 30 ml     |
| (6) Microplate (96-well)<br>Used in sample dilution or container for reaction<br>The plate is reusable after soaking in 1 % sodium hypochlorite<br>solution overnight.   | 1 plate   |

**IV. Materials Required but not Provided**

- Stop Solution : 0.5 N NaOH

Prepare Stop Solution prior to beginning the assay.

**Note:** This solution is corrosive. It may cause inflammation when it contacts skin.  
If it comes to contact with hands or mucous membranes, immediately wash  
away with a large amount of water and seek medical assistance.


**V. Storage**      4°C

## VI. Preparation of Reagents

1. All reagents should be brought to room temperature before use.
2. Preparation of substrate solution

Dissolve 1 vial (24 mg) of (1) pNPP (*p*-nitro-phenyl phosphate) Substrate in 5 ml of (4) ACP Buffer or (5) ALP Buffer, and use this as the Substrate Solution (substrate concentration : 12.5 mM). When used for tartrate-resistant acid phosphatase (TRACP), (3) Sodium Tartrate Solution should be added at 1/10 the volume of the Substrate Solution. In both cases, the prepared reagents should be stored at  $-20^{\circ}\text{C}$  , and used within 1 week.

## VII. Outline of Protocol

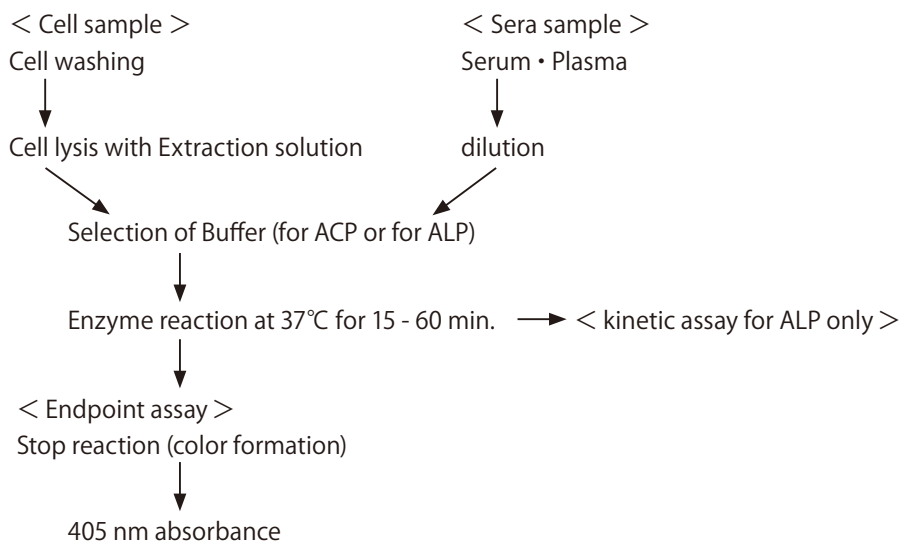

**VIII. Protocol****1. Adherent cells cultured in a 96-well plate**

- A. Remove the culture supernatant with an aspirator, etc.
- B. Add 200  $\mu$ l of physiological saline to each well, wash once, then discard the liquid.

**Note:**

- If the cells are detached, this process should be omitted, and a blank well containing medium only should be set to correct the observed data.
- Phosphate buffers should not be used in washing steps because they might inhibit the enzyme reaction.

- C. Pipetting lightly, add 5 - 50  $\mu$ l of (2) Extraction Solution to each well.

**Note:**

- The amount of Extraction Solution added can be changed depending on the number of cells. Approximately, 50  $\mu$ l should be used in the case of  $10^4$  cells.
- Sample should be diluted with (2) Extraction Solution when the sample concentration is high. (If Extraction Solution is insufficient, physiological saline can be substituted.)
- Part of the diluted sample (5 - 50  $\mu$ l) should be used in subsequent reactions.
- Lysis of the cells should be confirmed by microscopic observation.

- D. Add 50  $\mu$ l of the Substrate Solution for measurement (see Section VI. for reagent preparation) to each well and react at 37°C for 15 - 60 minutes.

**Note:**

- Reaction time can be set arbitrarily.
- The volume ratio of the cell lysis sample and Substrate Solution should be a maximum of 1 : 1. The cell lysis sample volume should be less than the Substrate Solution volume.
- If high enzyme activity is expected, it is recommended to prepare a diluted cell lysis solution for measurement in the provided 96-well plate.

- E. Add 50  $\mu$ l of Stop Solution (0.5 N NaOH) to each well and measure the absorbance at 405 nm after color formation.

**Note:**

- In the case of acid phosphatase, color formation starts with the addition of Stop Solution.
- Cell lysis sample obtained using the provided (2) Extraction Solution can be used for other measurements besides the target enzyme activity with this kit, such as protein quantification and kinase activities.

## 2. Suspension cells cultured in a Petri dish

- A. Collect culture medium with suspension cells into a tube and recover the cells by centrifugation.  
Wash the cells once with physiological saline and precipitate them by centrifuging again.
- B. Add 50 - 500  $\mu$ l of (2) Extraction Solution to each, and lyse the cells by pipetting.

**Note:**

- The amount of Extraction Solution added can be changed depending on the number of cells.
  - Roughly 50  $\mu$ l should be used for  $10^5$  cells and 500  $\mu$ l for  $10^7$  cells.
- C. Dilute the cell lysate step-wise with physiological saline and add the prescribed amount (in the range of 5 - 50  $\mu$ l) to each well of the provided 96-well plate.  
Following this step, the procedure is the same as in Section VIII.1D - E.

## 3. Serum samples

- A. Add 5 - 50  $\mu$ l of sera samples (serum or plasma) to each well.

**Note:** Sample should be diluted with (2) Extraction Solution.

Following this step, the procedure is the same as in Section VIII.1D - E.

## IX. Experimental Examples

### 1. Measurement of Alkaline Phosphatase (ALP)

This kit was used to measure ALP activity in cultured cells derived from human small intestine. At the same time, ALP staining was conducted using the fixation solution and insoluble substrate BCIP/NBT included in the TRACP & ALP Double-stain Kit (Cat. #MK300).

Method :

Suspension of human small intestine cells (Intestine 407) that were serially cultured in 10 % FCS/RPMI1640 medium was added to the first row of a 96-well plate. The plate was prepared up to the 11th row by 2 - fold dilution (No. of cells :  $1 \times 10^4$  in row 1,  $5 \times 10^3$  in row 2, and thereafter decreasing by half; row 12 was blank), then further cultured for 2 days (volume : 100  $\mu$ l/well). After culturing, ALP staining was conducted with insoluble substrate BCIP/NBT on columns A and B, and ALP activity was measured in columns C - F using this kit and protocol. Due to solubilization, the volume of (2) Extraction Solution added to columns C - F varied from 5 to 50  $\mu$ l (5  $\mu$ l in column C, 10  $\mu$ l in column D, 20  $\mu$ l in column E, 50  $\mu$ l in column F). Enzyme reactions were incubated for 60 minutes at 37°C.

Results :


Alkaline phosphatase activity is extremely strong in small intestine cells, and the correlation of activities and number of cells were confirmed using this kit. The detection sensitivity for human small intestine cells (Intestine 407) under the conditions of this activity measurement was 10 cells/assay. It was confirmed that even though the volume of (2) Extraction Solution added varied in the range of 5 - 50  $\mu$ l/well, there was little influence on the enzyme reactions. There is no problem in varying the volume of (2) Extraction Solution within a fixed range if the cells are solubilized at a sufficient volume.

Plate row		1	2	3	4	5	6	
	No. of cells (cells/well)	$1 \times 10^4$	$5 \times 10^3$	$2.5 \times 10^3$	$1.25 \times 10^3$	$6.25 \times 10^2$	$3.13 \times 10^2$	
A405 Plate Column	C	5 $\mu$ l *	2.275	2.271	1.732	0.920	0.581	0.329
	D	10 $\mu$ l *	2.298	2.263	1.957	1.082	0.719	0.373
	E	20 $\mu$ l *	2.289	2.273	1.901	1.101	0.617	0.369
	F	50 $\mu$ l *	2.236	2.214	1.964	1.287	0.744	0.341

\* : Volume of (2) Extraction Solution added

7	8	9	10	11	12
$1.56 \times 10^2$	$7.8 \times 10^1$	$3.9 \times 10^2$	20	10	0
0.239	0.180	0.160	0.158	0.154	0.145
0.252	0.200	0.176	0.154	0.158	0.148
0.228	0.192	0.168	0.162	0.152	0.145
0.234	0.175	0.161	0.152	0.157	0.145

### Staining of ALP. $1 \times 10^4$ cells /well

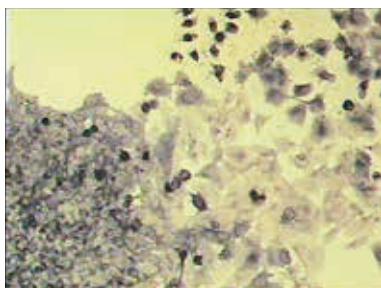

## 2. Measurement of Tartrate-resistant Acid Phosphatase (TRACP)

Method :

Bone marrow cells derived from the femur of a 16-week-old rabbit were suspended in 10 % FCS/RPMI1640 medium. This cell suspension was added to the first row of a 96-well plate, and the plate was prepared up to the 11th row by 2 - fold dilution of the same culture (No. of cells :  $7 \times 10^5$  in row 1,  $3.5 \times 10^5$  in row 2, and thereafter decreasing by half in the same manner; row 12 was blank), at a volume of 100  $\mu$ l/well, and culturing was initiated. A further 100  $\mu$ l of medium was added because adhesive cells had become prominent after 3 days, and culturing was continued. Eight days after seeding, TRACP activity was measured using the kit according to the protocol (Section VI).

The degree of substrate color formation was compared when substrate solution was directly added to the adhesive cells without extraction procedure and when they were solubilized with 25  $\mu$ l of extraction solution. 50  $\mu$ l of substrate solution for TRACP was used, and enzyme reactions were incubated for 60 minutes at 37°C.



## Results :

The bone marrow cell culture produces numbers of naturally differentiated osteoclast-like TRACP-positive cells, and their TRACP activity could be measured using this kit.

The table below shows the numbers of cells at the start of culturing and TRACP activity as absorbency at 405 nm. Similar levels of activity were detected in the live cells to which substrate was directly added without extraction (final substrate concentration 12.5 mM) and in cells on which extraction was conducted (final substrate concentration 4.1 mM), and results that correlated with the numbers of cells were obtained.

No. of cells (cells/well)	$7 \times 10^5$	$3.5 \times 10^5$	$1.75 \times 10^5$	$8.76 \times 10^4$	$4.38 \times 10^4$	$2.19 \times 10^4$
Substrate directly added	1.701	1.471	0.747	0.295	0.156	0.120
Extracted	1.754	1.880	0.781	0.246	0.150	0.125

$1.1 \times 10^3$	$5.5 \times 10^2$	$2.25 \times 10^2$	112	56	0
0.105	0.100	0.104	0.102	0.100	0.100
0.112	0.111	0.112	0.107	0.105	0.108

### 3. Measurement with Acid Phosphatase (ACP) Standards

## Method :

A standard curve was made using ACP (Code. 108227, Lot 93207721) from Roche Diagnostics.

Distilled water was added to the reference standards to prepare 100  $\mu\text{g/ml}$  enzyme solutions, and a 2 - fold dilution series was prepared using each enzyme buffer.

Using 1 well of a 96-well plate for 1 reaction, 50  $\mu\text{l}$  of enzyme and 50  $\mu\text{l}$  of the Substrate Solution were mixed and reacted for 30 minutes at 37°C. After adding 50  $\mu\text{l}$  of Stop Solution, absorbency at 405 nm was immediately measured using a plate reader.

**Note:**


- In the case of acid phosphatase, color forms with the addition of Stop Solution.
- Tartaric acid is not added to acid phosphatase substrate.

## Results :

For ACP, concentrations were measurable from 1.5  $\mu\text{g/ml}$  or less, and linearity was obtained in the range up to 0.5  $\mu\text{g/ml}$ .

Acid phosphatase 100  $\mu$ l/ml preparation :  $2^1 - 2^{15}$  stepwise dilution

$\mu$ l/ml	405 nm
50	4.014
25	3.993
12.5	3.995
6.26	4.066
3.125	4.011
1.5625	4.032
0.78125	3.411
0.390625	2.043
0.195313	1.147
0.097656	0.599
0.048828	0.356
0.024414	0.215
0.012207	0.157
0.006104	0.120
0.003052	0.108
0	0.084

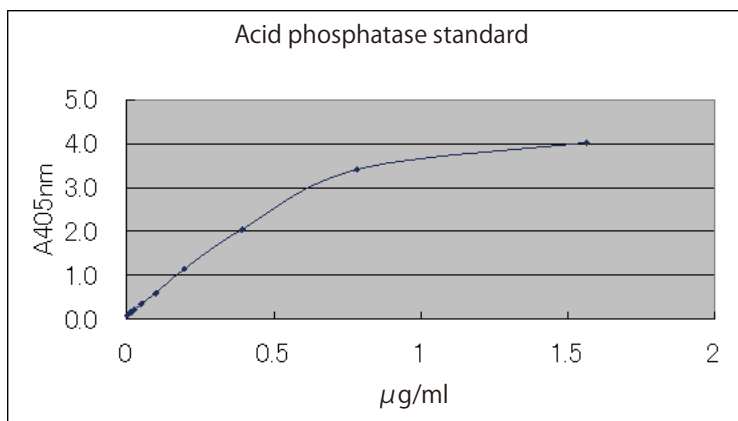

**4. Measurement with Alkaline Phosphatase (ALP) as standard sample**

Method :




A standard curve was made using 3 types of alkaline phosphatase (ALP), BAP (Cat. #2120A, Lot K2601EA), CIAP (Cat. #2250A, Lot E2301AB), or SAP (Cat. #2660A, Lot N301CB).

Each enzyme was diluted with (2) Extraction Solution to prepare the enzyme solution at highest concentration. Then the enzyme solutions at 2-fold serial dilution were prepared using (5) Buffer for ALP. Both 50  $\mu$ l of enzyme solution and 50  $\mu$ l of pNPP substrate dissolved in the (5) Buffer for ALP were added and mixed in one well of a 96-well plate, and incubated at 37°C for 30 minutes. Immediately after adding 50  $\mu$ l of Stop Solution, absorbance at 405 nm of the 96-well plate was measured using a micro plate reader.

Result :

All 3 alkaline phosphatases were available as a positive control.

BAP		CIAP		SAP	
$\mu$ U/ $\mu$ l	405 nm	$\mu$ U/ $\mu$ l	405 nm	$\mu$ U/ $\mu$ l	405 nm
2000	4.000	8500	4.000	10000	4.000
1000	4.000	4250	4.000	5000	4.000
500	4.000	2125	4.000	2500	4.000
250	4.000	1062.5	4.000	1250	4.000
125	4.000	531.25	4.000	625	4.000
62.5	4.000	265.63	4.000	312.5	4.000
31.25	2.351	132.81	4.000	156.25	3.020
15.63	1.333	66.41	3.657	78.13	1.777
7.81	0.749	33.2	2.168	39.06	1.025
3.92	0.422	16.6	1.207	19.53	0.583
1.95	0.252	8.3	0.650	9.77	0.337
0.98	0.165	4.15	0.376	4.88	0.216
0.49	0.123	2.08	0.231	2.44	0.151
0.24	0.104	1.04	0.162	1.22	0.120
0.12	0.098	0.52	0.126	0.61	0.101
0	0.087	0	0.087	0	0.084

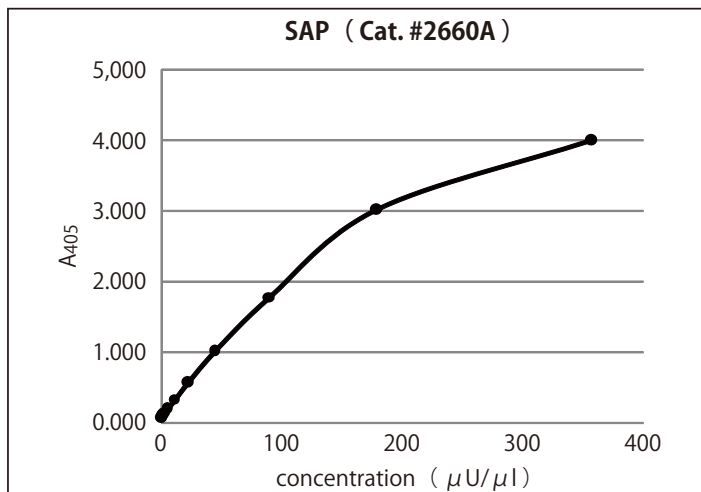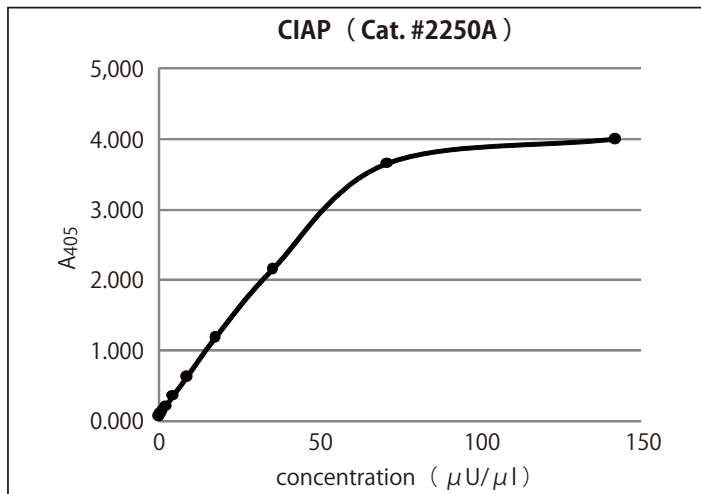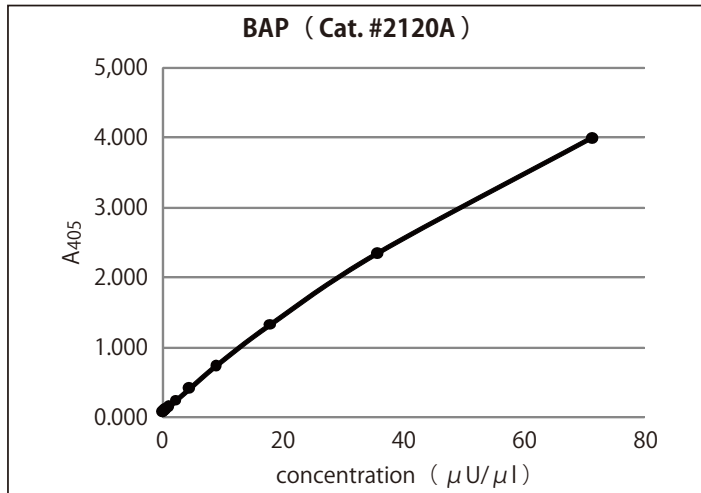

**5. Comparison of Tartrate-resistant Acid phosphatase (TRACP) and Alkaline Phosphatase (ALP) by the preparation method of sera samples.**

Method :

Blood was collected from three rabbits simultaneously and the collected sera samples were prepared by three methods (citrate plasma (PPP), serum and hemolysis serum). 50  $\mu$ l of serial dilution samples and 50  $\mu$ l of the respective substrate solution were mixed and reacted for 30 minutes at 37°C. After adding 50  $\mu$ l of Stop Solution, absorbance at 405 nm was measured using a plate reader. All of the samples were measured simultaneously on the day when serum samples were prepared.

Results :

< TRACP activity >							A405 nm absorbance		
TRACP	citrate plasma (PPP)			serum			hemolysis serum		
ID No.	20X	40X	80X	20X	40X	80X	20X	40X	80X
Rb No. 1	0.821	0.420	0.247	0.834	0.487	0.309	0.834	0.487	0.300
Rb No. 2	1.045	0.520	0.311	0.704	0.422	0.268	1.066	0.582	0.360
Rb No. 3	0.702	0.370	0.237	1.000	0.579	0.353	0.768	0.360	0.275

< ALP activity >							A405 nm absorbance		
ALP	citrate plasma (PPP)			serum			hemolysis serum		
ID No.	2X	4X	8X	2X	4X	8X	2X	4X	8X
Rb No. 1	0.514	0.321	0.217	0.801	0.469	0.295	1.074	0.599	0.374
Rb No. 2	0.481	0.299	0.206	0.528	0.327	0.217	0.801	0.483	0.304
Rb No. 3	0.348	0.231	0.165	0.718	0.431	0.275	0.650	0.398	0.252

As the phosphatase activity is different depending on the preparation method of blood sample, it is necessary to use the sample of the same preparation method.

**6. Effect of freeze-thaw cycles of serum samples on phosphatase activity.**

Method :

Serum samples were collected from three rabbits. Samples were divided into four portions and each sample was repeated various cycles of freeze-thawing ( $-80^{\circ}\text{C} \leftrightarrow 25^{\circ}\text{C}$ ). For the measurement of TRACP (tartrate-resistant acid phosphatase), samples were diluted by 20-, 40- and 80-fold. For the measurement of ALP (alkaline phosphatase), samples were diluted by 2-, 4- and 8-fold.

50  $\mu$ l of serial dilution samples and 50  $\mu$ l of the respective substrate solution were mixed and reacted for 30 minutes at 37°C. After adding 50  $\mu$ l of Stop Solution, absorbance at 405 nm was measured using a plate reader. All of the samples were measured simultaneously on the day when serum samples were prepared.

Results :

&lt; TRACP activity &gt;

A405 nm absorbance

TRACP	no freezing			freeze-thaw 1 cycle			freeze-thaw 2 cycles			freeze-thaw 3 cycles		
ID No.	20X	40X	80X	20X	40X	80X	20X	40X	80X	20X	40X	80X
Rb No. 1	0.826	0.477	0.295	0.832	0.438	0.284	0.778	0.452	0.292	0.736	0.432	0.277
Rb No. 2	1.087	0.577	0.342	1.078	0.573	0.343	1.021	0.580	0.353	0.980	0.565	0.344
Rb No. 3	0.743	0.409	0.252	0.754	0.429	0.269	0.749	0.434	0.279	0.710	0.424	0.275

&lt; ALP activity &gt;

A405 nm absorbance

ALP	no freezing			freeze-thaw 1 cycle			freeze-thaw 2 cycles			freeze-thaw 3 cycles		
ID No.	2X	4X	8X	2X	4X	8X	2X	4X	8X	2X	4X	8X
Rb No. 1	0.616	0.338	0.281	0.602	0.328	0.212	0.592	0.335	0.214	0.588	0.330	0.221
Rb No. 2	0.577	0.327	0.206	0.600	0.338	0.214	0.562	0.324	0.209	0.577	0.334	0.213
Rb No. 3	0.400	0.243	0.164	0.423	0.255	0.170	0.440	0.261	0.175	0.415	0.248	0.173

It appeared that both TRACP and ALP activities were not strongly influenced by freeze-thaw cycles of sera samples, but it was preferable to limit to 2 freeze-thaw cycles.

## X. References

- 1) Burstone, M. S. *et al.* (1958) *J Natl Cancer Inst.* **20**, 601-615.
- 2) Burstone, M. S. *et al.* (1958) *J Natl Cancer Inst.* **21**, 523-539.
- 3) Burstone, M. S. (1959) *J Histochem Cytochem.* **7**, 39-41.
- 4) Harlow and Lane (1988) *Antibodies, A LABORATORY MANUAL.* 406-407.

## XI. Related Products

TRACP & ALP double-stain Kit (Cat. #MK300)  
 Alkaline Phosphatase (*E. coli* C75) (BAP) (Cat. #2120A)  
 Alkaline Phosphatase (Calf intestine) (CIAP) (Cat. #2250A)  
 Alkaline Phosphatase (Shrimp) (SAP) (Cat. #2660A)

**NOTE :** This product is for research use only. It is not intended for use in therapeutic or diagnostic procedures for humans or animals. Also, do not use this product as food, cosmetic, or household item, etc.

Takara products may not be resold or transferred, modified for resale or transfer, or used to manufacture commercial products without written approval from TAKARA BIO INC.

If you require licenses for other use, please contact us by phone at +81 77 565 6973 or from our website at [www.takara-bio.com](http://www.takara-bio.com).

Your use of this product is also subject to compliance with any applicable licensing requirements described on the product web page. It is your responsibility to review, understand and adhere to any restrictions imposed by such statements.

All trademarks are the property of their respective owners. Certain trademarks may not be registered in all jurisdictions.